

# PHILIPS

Mother & Child Care

ECG monitoring



## A fetal monitoring solution designed around you

### Fetal direct ECG monitoring

Philips spiral electrodes are designed for easy and safe use. Plus, our uniquely designed fetal direct ECG (DECG) Reusable Legplate Adapter Cable makes cleaning more accessible than ever.

Every part of the system – the Fetal Spiral Electrode, DECG Reusable Legplate Adapter Cable and disposable Attachment Electrode – has been designed around the way you work.


The handle features a protection tab that keeps the spiral tip inside the tube during insertion. This feature is intended to prevent accidental puncture to the mother's birth canal, the fetus or your fingertips. The protection tab also serves as a visual reference point to indicate how far the spiral has turned when attaching the electrode.

In addition, a simple connector plugs securely into the legplate adapter cable to deliver accurate, reliable fetal heart rate readings.



Fetal Spiral Electrode

Fetal Double-Spiral Electrode

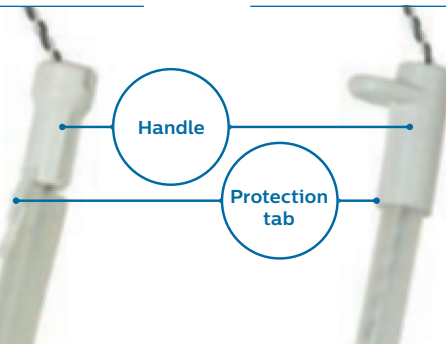

## Simple to clean

An improved legplate adapter cable is a one-piece, seamless design. The electronics are completely sealed, so you can safely immerse it in most cleaning and disinfection fluids. The Attachment Electrode connection socket is also sealed, so body fluids are less likely to enter during monitoring. Finally, a convenient flushing port makes it more accessible to clean the inside of the connector if needed. The Philips system is truly a great solution.


## A versatile performer

Philips fetal monitoring system has been tested and verified to deliver accurate signals and performance with Philips fetal monitors.

It's all part of Philips commitment to bringing you the most advanced technology built to the highest standards of quality.

## Fast cleaning

A convenient flushing port allows you to wash out the inner chamber.

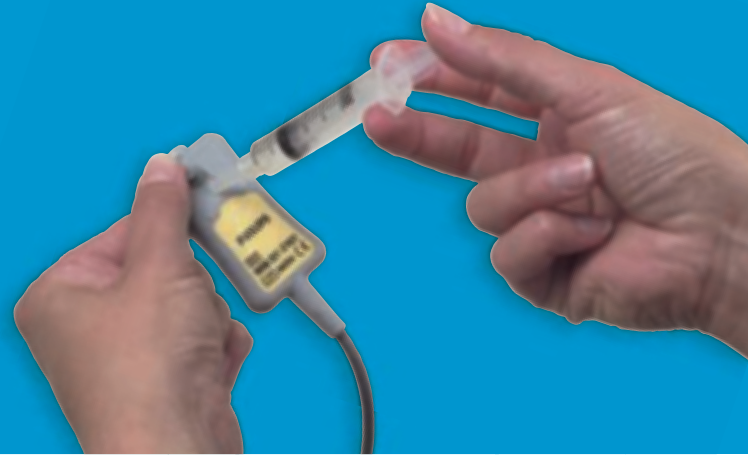







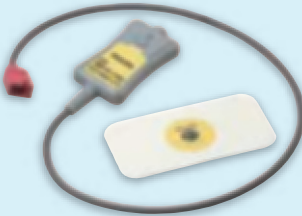


DECG Reusable Legplate Adapter Cable 989803137651  
and Attachment Electrode 989803139771




Fetal Spiral Electrode  
989803137631

# Component setup

These monitors ...	... connect to ...	... with either of these spiral electrodes
Philips and legacy Hewlett-Packard/Agilent monitors	 <p>Avalon patient module M2738A</p>	Fetal Spiral Electrode 989803137631 <b>or</b> Fetal Double-Spiral Electrode* 989803137641
	 <p>Toco+ transducer M2735A</p>	
	 <p>CL Toco+ MP transducer 866075</p>	
	 <p>CL ECG/IUP transducer 866077</p>	
	 <p>Avalon Toco+ MP transducer 867245</p>	
	 <p>Avalon ECG/IUP transducer 867247</p>	
	 <p>Avalon Toco+ transducer 867249</p>	
	 <p>DECG Reusable Legplate Adapter Cable 989803137651</p> <p>Attachment Electrode 989803139771</p>	

\* Not all transducers and Fetal Scalp Electrodes are available in all countries.



 Philips Medical Systems  
3000 Minuteman Road  
Andover, MA 01810 USA

© 2020 Koninklijke Philips N.V. All rights are reserved.  
Philips reserves the right to make changes in specifications and/or to discontinue any product at any time without notice or obligation and will not be liable for any consequences resulting from the use of this publication. Trademarks are the property of Koninklijke Philips N.V. or their respective owners.

[www.philips.com](http://www.philips.com)

Printed in the Netherlands.  
4522 991 58661 \* SEP 2020